


Supplemental Figure S31A. Meta-analysis for Experience with speaking rate of each device.

Supplemental Figure S31B. Meta-analysis for Skin irritation rate of each device.

Meta-analysis for experience with speaking among different voice prosthesis in laryngectomized patients

A

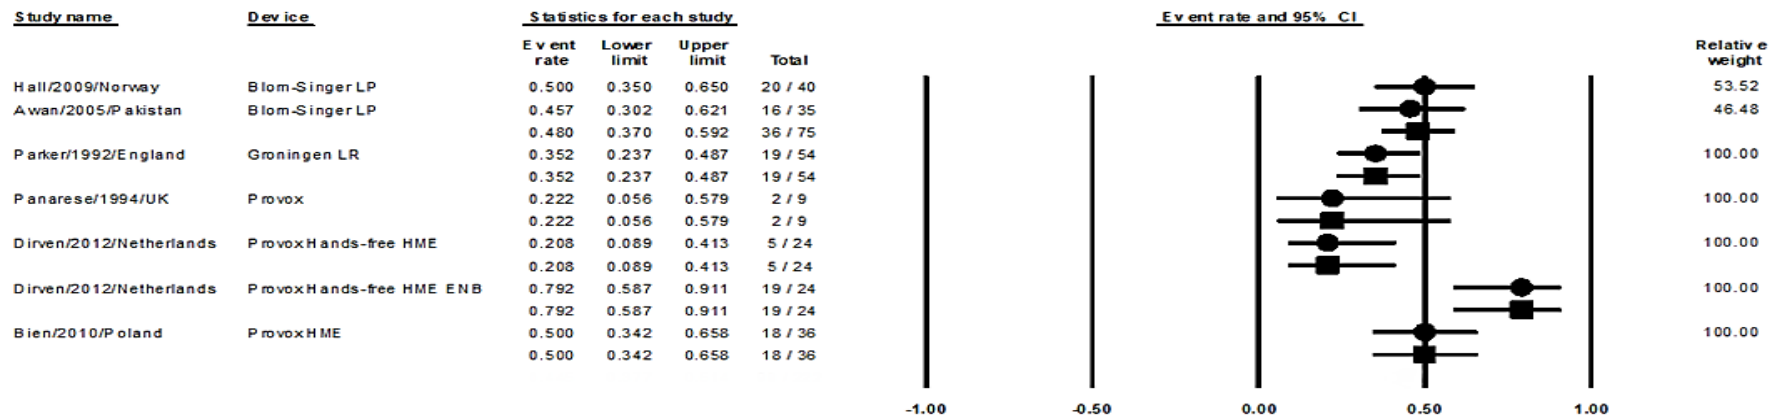

B

Meta-analysis for skin irritation among different voice prosthesis in laryngectomized patients

